



# UV config - CST FSC DIODE PE 561 - 2B 6V 4YG 2UV 3R

Cytometer:	LSRFortessa	User:	Administrator
Cytometer Name:	LSRFortessa	Institution:	N/A
Serial Number:	1	Software:	BD FACSDiva 8.0.1
Input Device:	Manual	Date:	9/8/2016 2:31:22 PM
Window Extension:	10.00		


Blue Laser  
(488nm)  
FSC

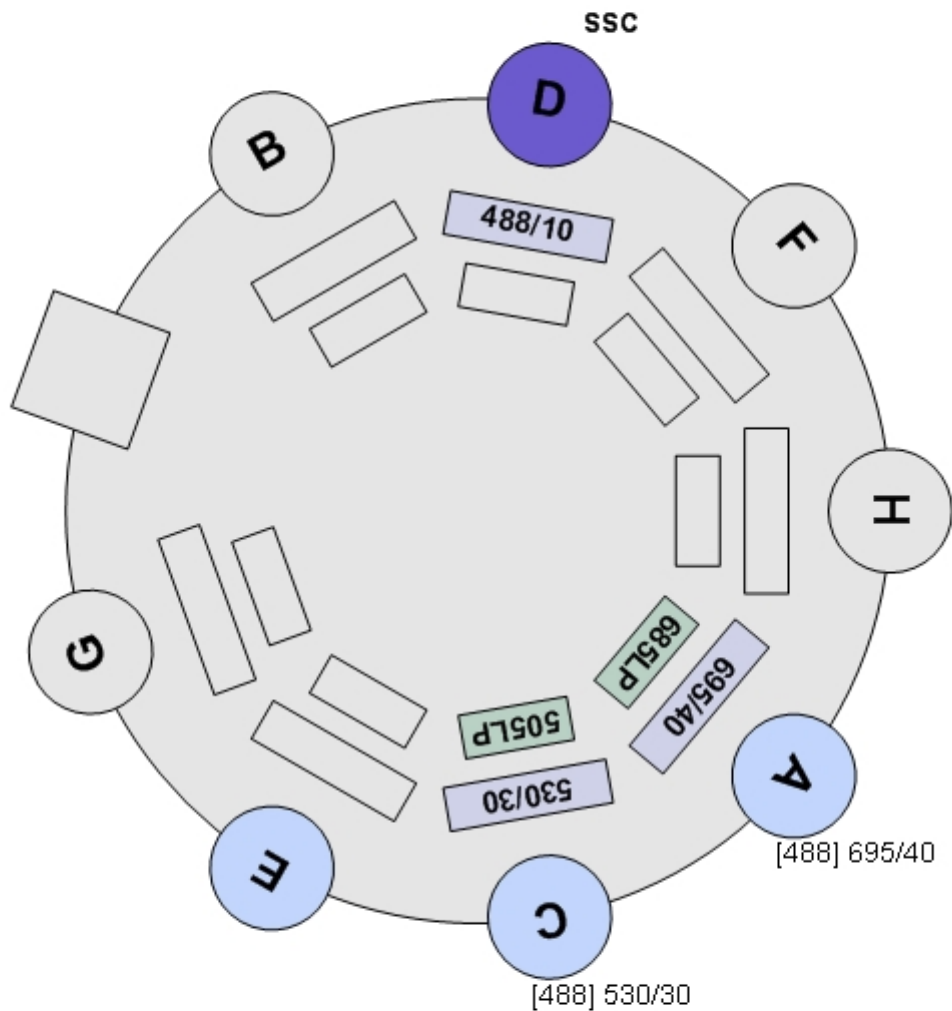


Red Laser  
(640nm)

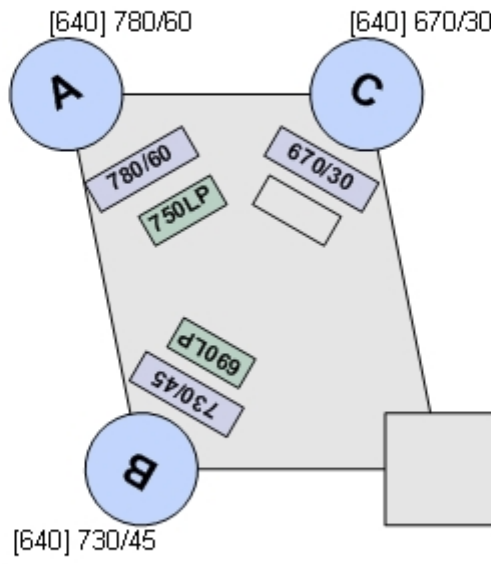


Violet Laser  
(405nm)

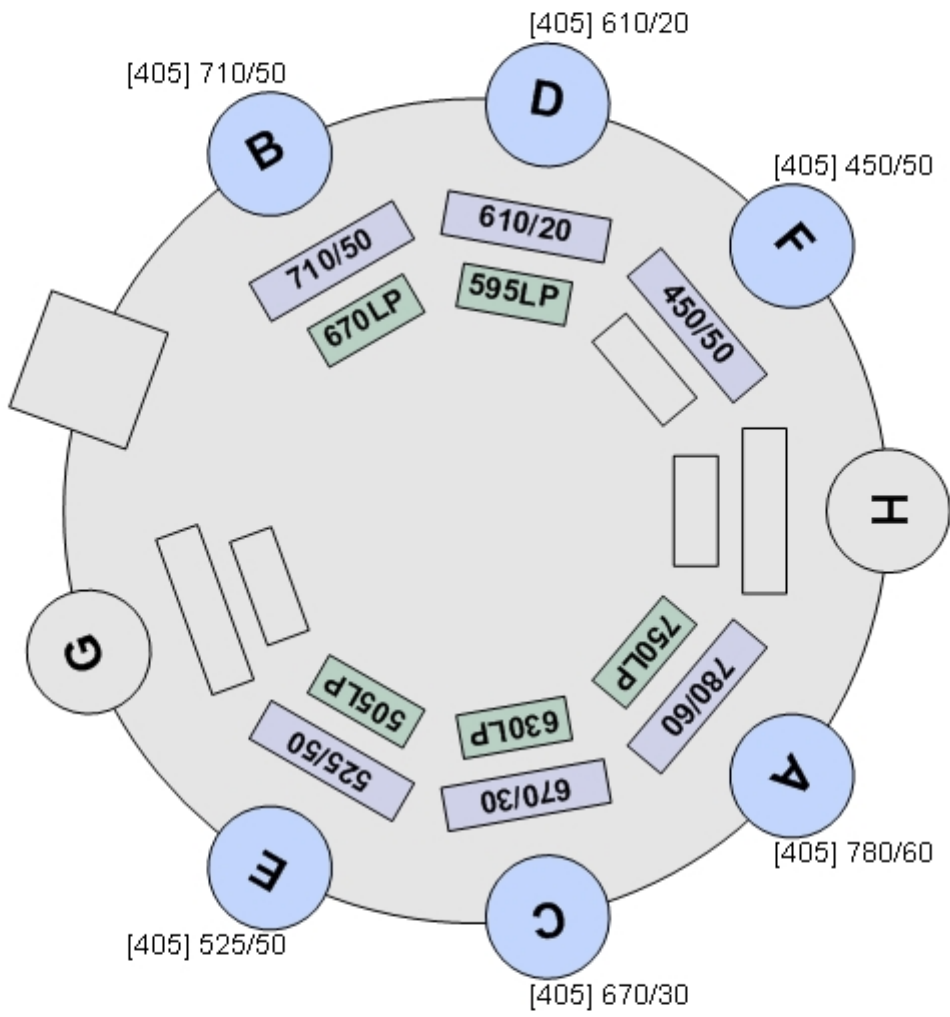

UV Laser  
(355nm)

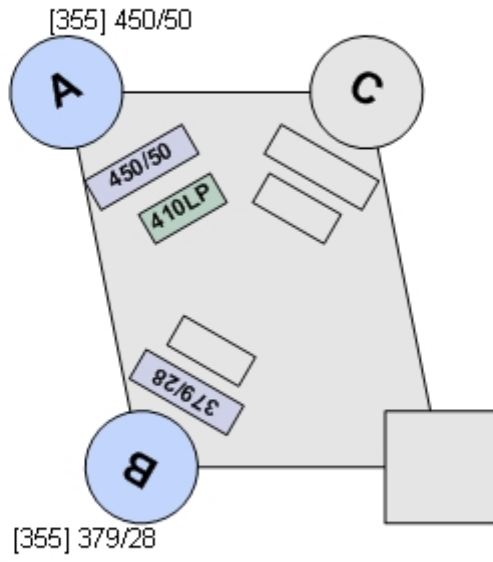

**Yel-Gr Laser  
(561nm)**

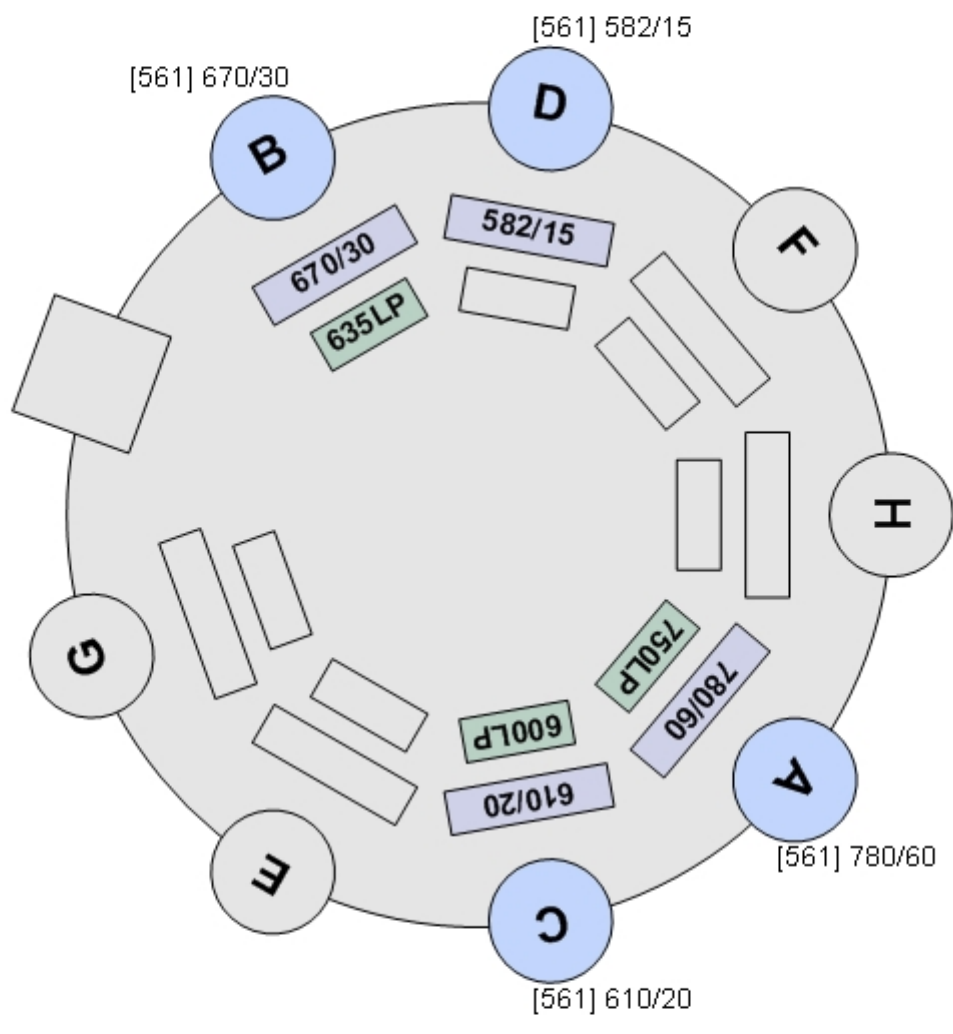

Comments:

Configuration setup for use with BUV395 and LiveDead UVEFl455