



CMCA_PC2 Jan 2017 New (4-2-2)


Cytometer:	FACSCantoII	User:	Maintenance
Cytometer Name:	FACSCantoII	Institution:	Curtin
Serial Number:	V96100173	Software:	BD FACSDiva 8.0.1
Input Device:	HTS	Date:	01/02/2017 8:30:16 AM
Window Extension:	7.00		

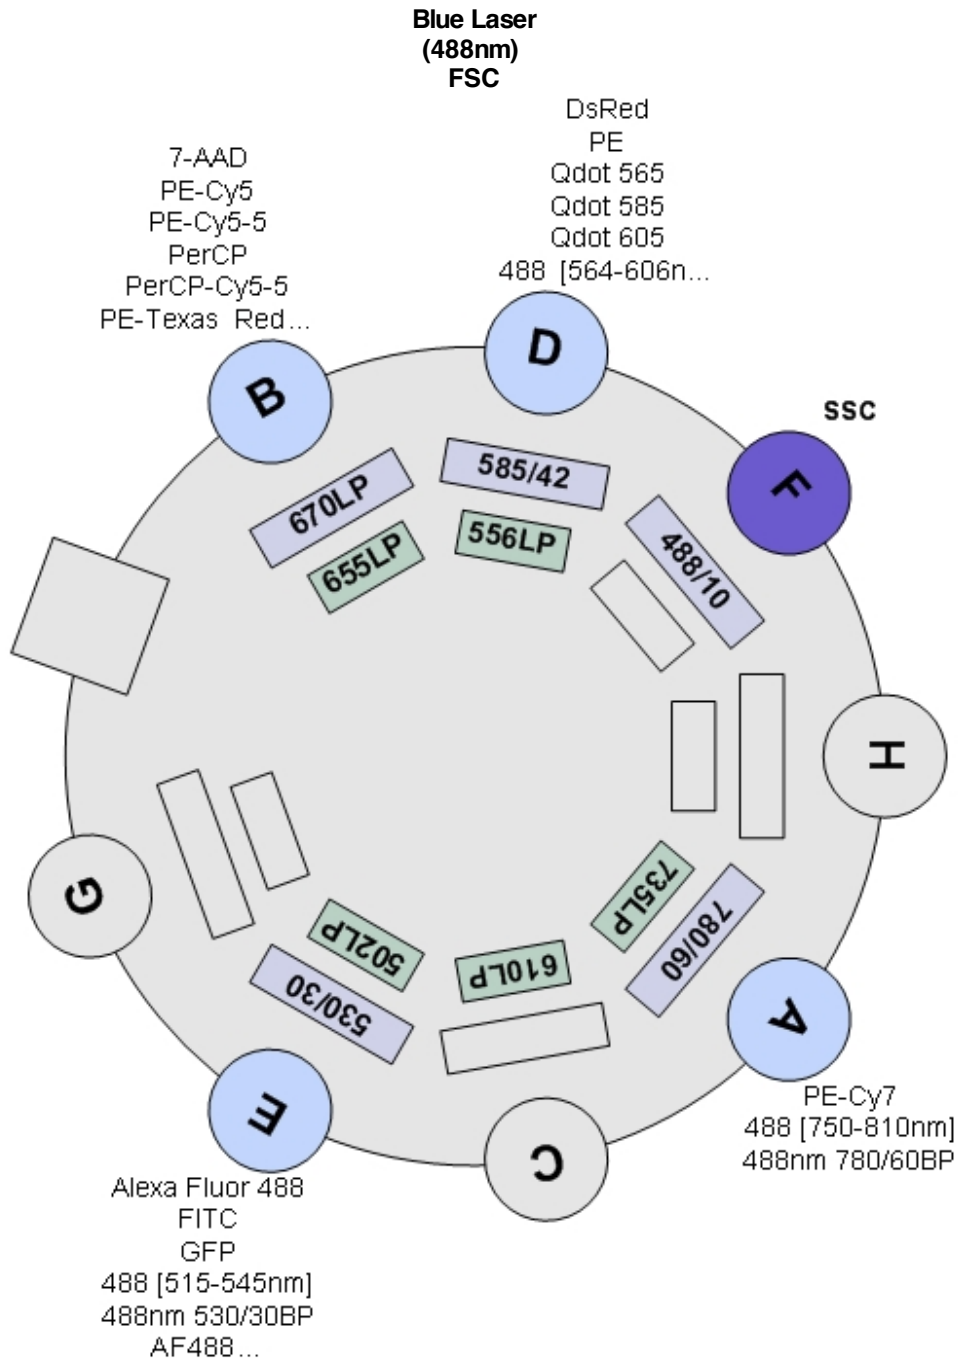

**Red Laser
(633nm)**

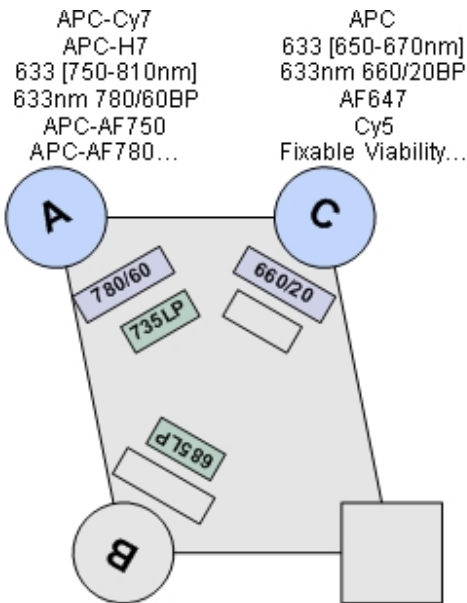

**Violet Laser
(405nm)**

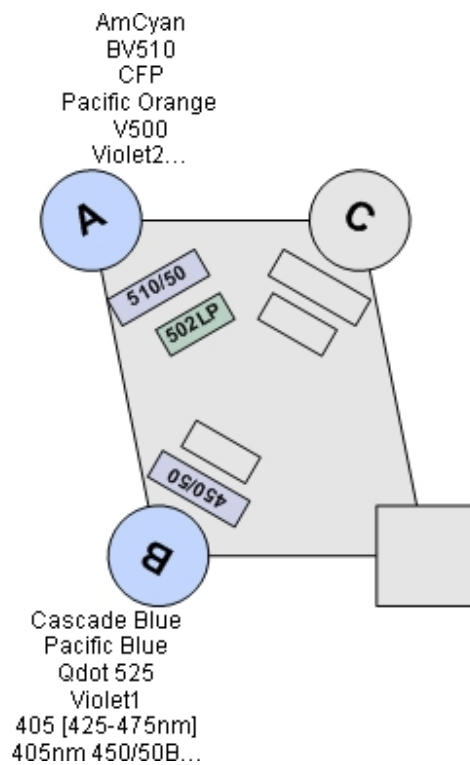

Comments: